

204710" T590500T

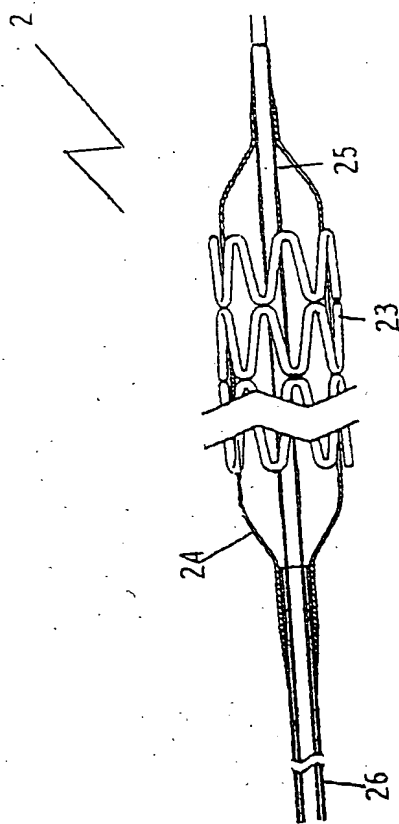
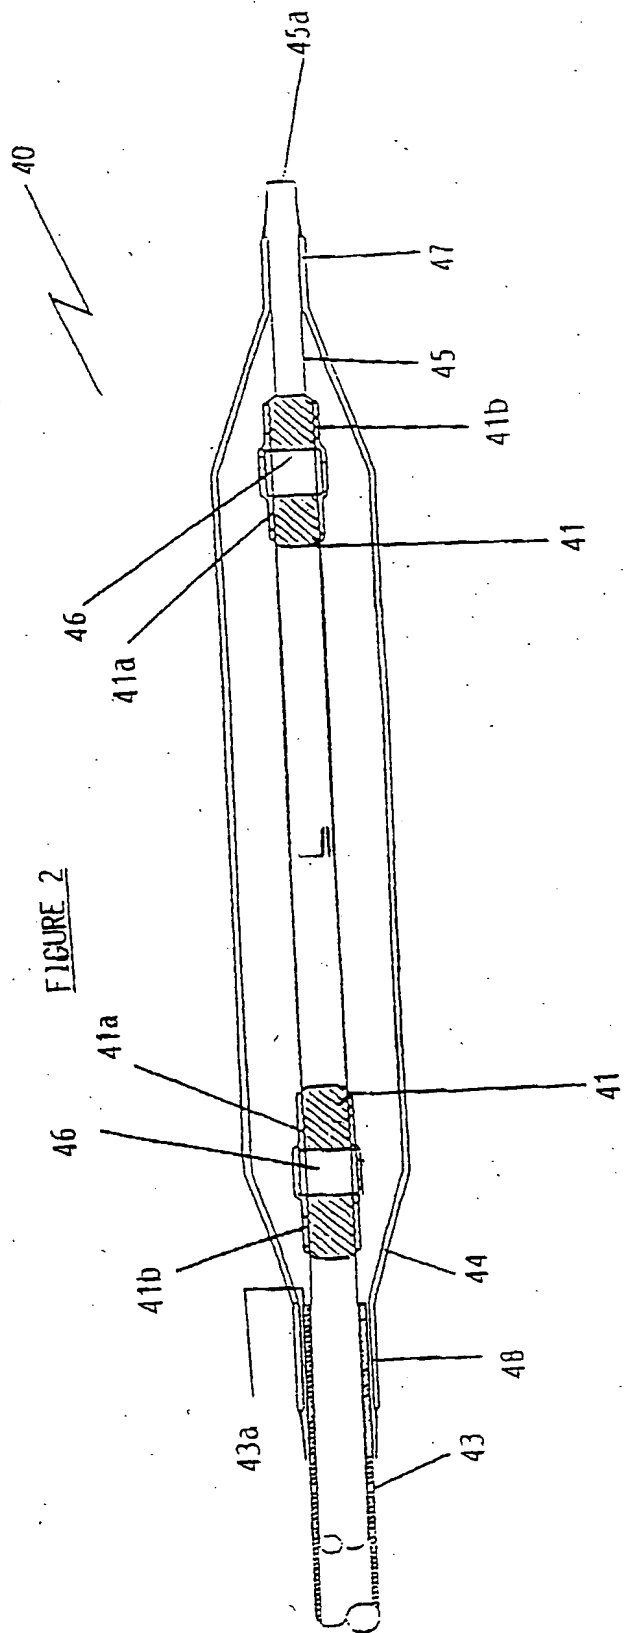


FIGURE 1



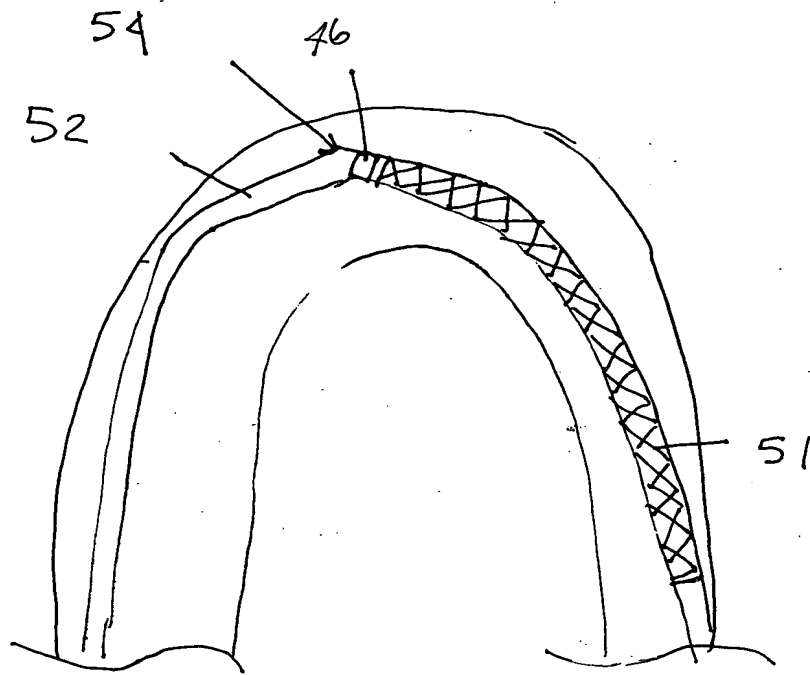


Fig. 3a

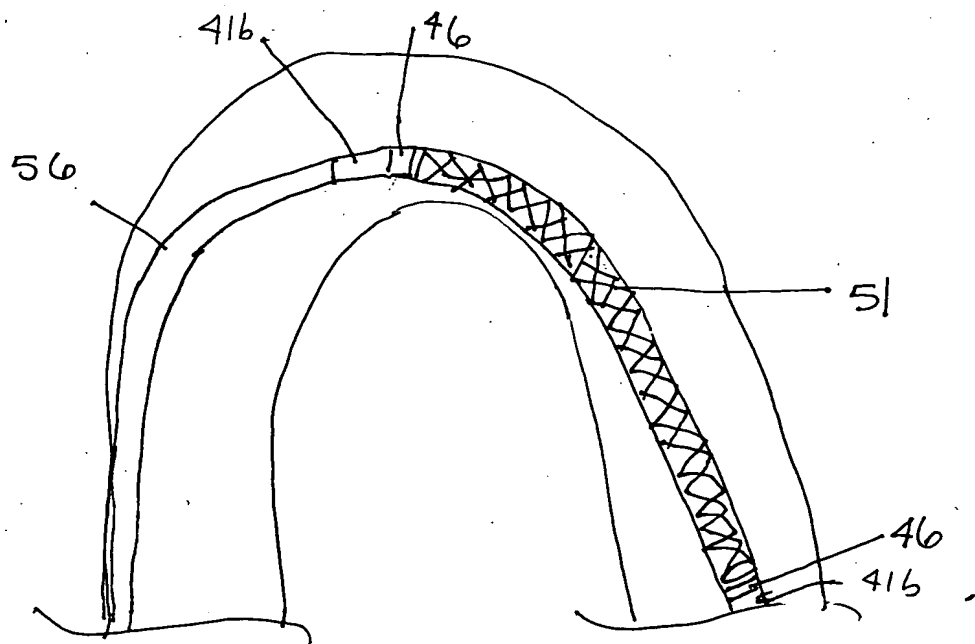


Fig. 3b

Figure 4 90° Fixed Wire Track Profile for a stent delivery system without areas of increased stiffness proximal and distal to the stent with respect to the flexible catheter.

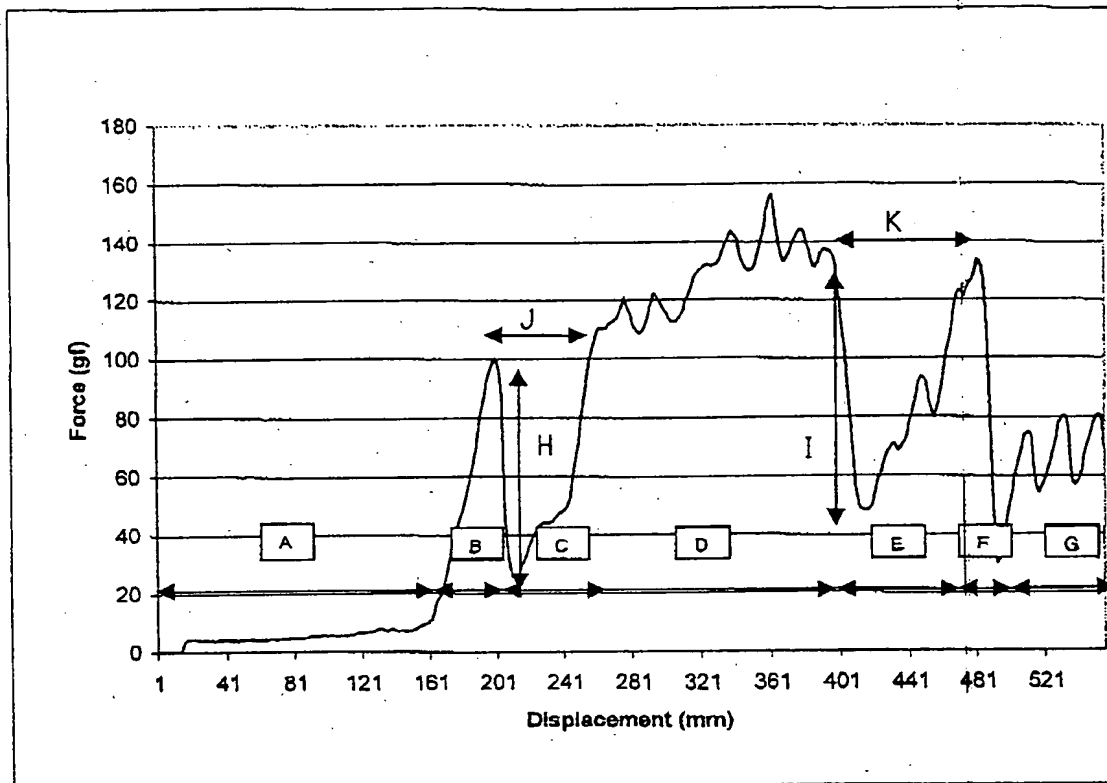


Figure 5 Track profile of stent delivery system with and without areas of increased stiffness Proximal and distal to the stent with respect to the flexible catheter

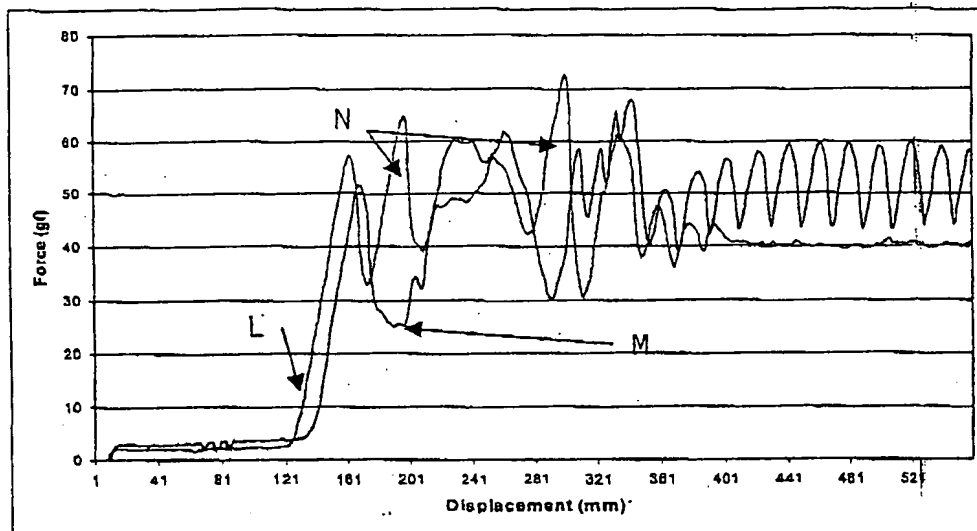


Figure 6 Track profile of 4.0x18 stent delivery system with and without areas of increased stiffness proximal and distal to the stent with respect to the flexible catheter

